


Moisture meter

Operating Manual

humimeter RH6


Paper moisture meter with sword sensor
for measuring the relative air humidity of paper

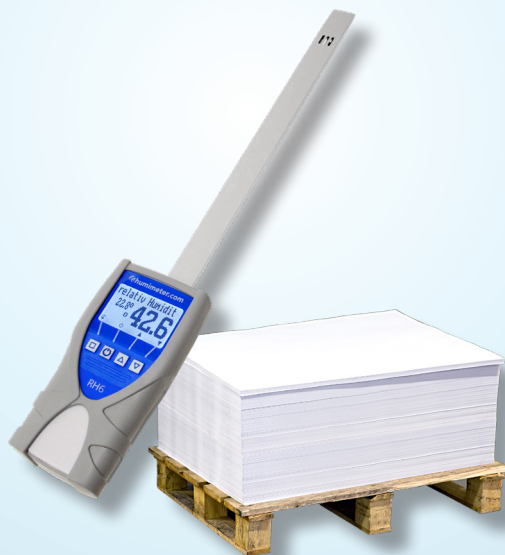

78,0 °F | 6,16% | 456kg/m³ | -27,3td | 0,64aw | 51,9%r.H. | 14,8%abs | 100,4g/m² | 09m/s | 4,90Ug/L | 1


Your humimeter RH6 at a glance

The main unit

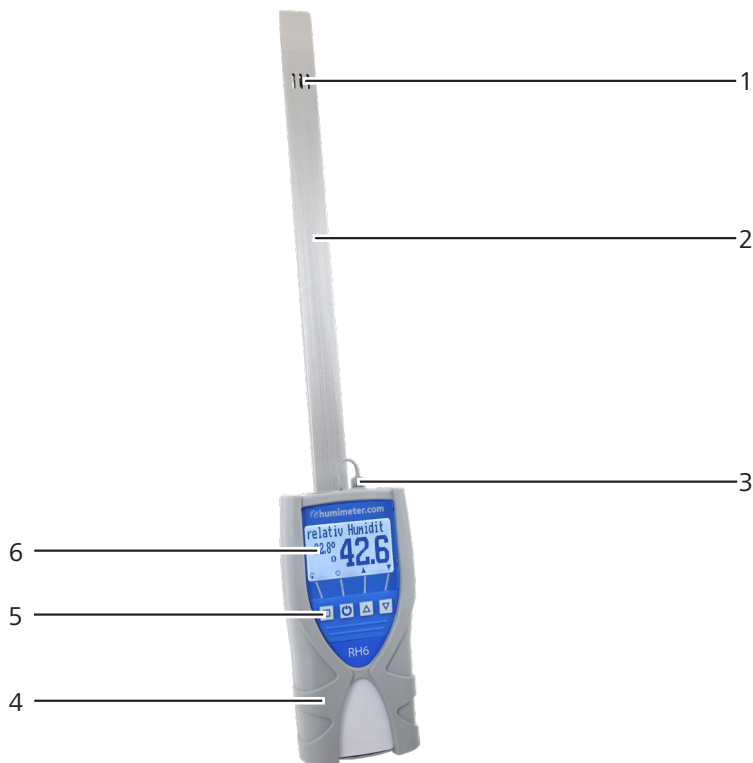

No.	Name
1	Air humidity and temperature sensor
2	Sword sensor
3	USB Port
4	Rubber protection cover
5	Keypad
6	Display

Rear of the main unit

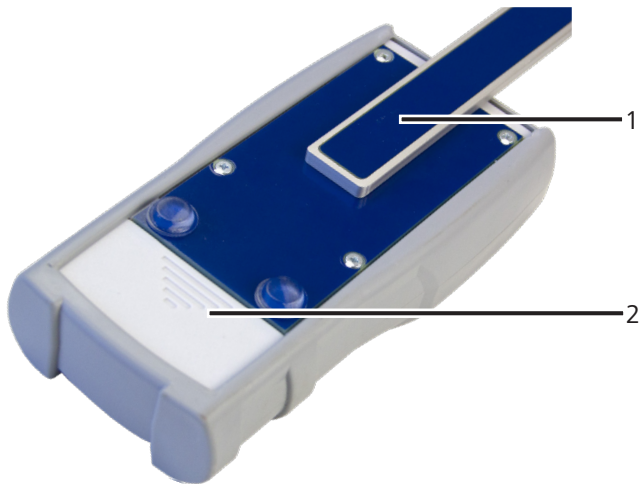





















No.	Name
1	Sword sensor
2	Battery compartment

The display



No.	Name
1	Product type
2	Relativ air humidity in % (see "7.1 Definition product types")
3	Display symbols
4	Temperature display

The display symbols

Symbol	Name	Symbol	Name
	Enter		No
	Up		Change input level
	Down		OK
	Back		Change menu
	Enter numbers		Enter data
	Enter letters		View measurements
	Continue / go right		Delete measurements
	Left		On/off button, display light
	Yes		Save measured value
	Auto save		Hold function

The menus

The device has three different menus: product selection, Data Log and main menu:

Product selection menu



No.	Name
1	Change menu
2	Display illumination / device on/off
3	For changing the product type

Data Log menu



No.	Name
1	Change menu
2	Display illumination / device on/off
3	Save measured value
4	Show the last recorded values

Main menu

The main menu comprises the following menu items:

- **Edit Logs:**
Manual Logs, Auto Logs, Clear Logs
- **Print Logs:**
Last Log, All Logs, Clear Logs
- **Send Logs:**
Manual Logs, Auto Logs, Clear Logs
- **Options:**
Bluetooth, Date/Time, Log Time, Language, Unlock, °C/°F, BL On Time, Auto Off Time, Calibrate, Materialcalibration, Online Send, Password, Reset
- **Status**

Table of contents

Your humimeter RH6 at a glance	2
The main unit	2
Rear of the main unit	3
The display	3
The display symbols	4
The menus	4
1. Introduction	9
1.1 Information about this operating manual	9
1.2 Limitation of liability	9
1.3 Symbols used in this manual	10
1.4 Customer service	10
2. For your safety	11
2.1 Proper use	11
2.2 Improper use	11
2.3 User qualifications	11
2.4 General safety information	12
2.5 Warranty	12
3. On receipt of your device	12
3.1 Taking the device out of its packaging	12
3.2 Making sure that all of the components have been included	12
3.3 Inserting batteries	13
4. Using the device - Basics	14
4.1 Switching the device on	14
4.2 Selecting the product type	14
4.3 Taking a measurement	14
4.4 Switching the device off	14
5. The measuring process	15

5.1	Taking a measuring at a stack	15
5.1.1	Taking a measurement of single pieces	16
5.2	Adjustment behaviour of the sensor	17
6.	Saving your readings	18
6.1	Hold function - Freezing the displayed values	18
6.1.1	Activating the Hold function in the Options menu	18
6.1.2	Using the Hold function	18
6.2	Saving your readings manually	19
6.2.1	Saving individual readings	19
6.2.2	Saving several readings (a measurement series) at the same time	21
6.3	Auto save function (time-based)	22
6.3.1	Activating the Auto save function in the Options menu	22
6.3.2	Auto save function: Saving measured values	22
6.4	Viewing individual readings	23
6.5	Viewing individual readings from a series of measurements	24
6.6	Deleting all measured values (data log)	24
6.7	Deleting individual measurement series	25
6.8	Deleting individual values from a single series of measurements	26
7.	Product types	27
7.1	Definition product types	27
7.2	Application range	28
8.	Using the LogMemorizer program	29
8.1	Installing/Opening the program	29
8.2	Exporting measured values to a computer	29
9.	Checking the device's status	32
10.	Configuring the device	32
10.1	Turning on Bluetooth	32
10.2	Adjusting the date/time	32
10.3	Selecting a language	33

10.4	Activating options	34
10.5	Deactivating options	35
10.6	Selecting °C/°F	35
10.7	Reducing the device's power consumption	35
10.7.1	Configuring the display illumination time	35
10.7.2	Configuring automatic switch-off	36
10.8	Calibrating the device	36
10.9	Configuring the material calibration function	36
10.10	Changing the password	36
10.11	Resetting the device to its factory settings	37
11.	Cleaning and maintenance	38
11.1	Changing the batteries	38
11.2	Care instructions	38
11.3	Cleaning the device	38
12.	2-point (optionally 3-point) calibration	39
12.1	Assembling the calibration equipment	39
12.2	Determining the deviation	40
12.3	Performing a recalibration	41
12.3.1	Determination of calibration values	41
12.3.2	Entering the calculated calibration values into the RH6	42
13.	Faults	44
14.	Storage and disposal	45
14.1	Storing the device	45
14.2	Disposing of the device	45
15.	Device information	46
15.1	EC declaration of conformity	46
15.2	Technical data	47

1. Introduction

1.1 Information about this operating manual

This operating manual is designed to enable you to use the humimeter RH6 safely and effectively. It is part of the device, has to be stored nearby and must be easily accessible to users at all times.

All users are required to carefully read and make sure that they have understood this operating manual before using the humimeter RH6. All of the safety and operating instructions detailed in this manual have to be observed to ensure the safety of the device.

1.2 Limitation of liability

All of the information and instructions provided in this operating manual have been compiled on the basis of the current standards and regulations, the state of the art, and the extensive expertise and experience of Schaller GmbH.

Schaller GmbH does not accept any liability for damage associated with the following, which also voids the warranty:

- Non-observance of this operating manual
- Improper use
- Inadequately qualified users
- Unauthorised modifications
- Technical changes
- Use of unapproved spare parts

This fast measuring procedure can be affected by a range of different factors.

We, as the manufacturer, do not accept any liability for any incorrect measurements and associated consequential damage.

1.3 Symbols used in this manual

All of the safety information provided in this manual is shown with a corresponding symbol.



ATTENTION

It is essential to observe this warning. Non-compliance can lead to damage to property or equipment.



Information

This symbol indicates important information that enables users to use the device more efficiently and cost-effectively.

1.4 Customer service

For technical advice, please contact our customer service department at

Schaller GmbH

Max-Schaller-Straße 99
A - 8181 St.Ruprecht an der Raab



Telephone: +43 (0)3178 28899
Fax: +43 (0)3178 28899 - 901

E-mail: info@humimeter.com
Internet: www.humimeter.com

© Schaller GmbH 2019

2. For your safety

The device complies with the following European directives:

- Restriction of Hazardous Substances in Electrical and Electronic Equipment (RoHS)
- Electromagnetic compatibility (EMC)

The device corresponds to state-of-the-art technology. However, it is still associated with a number of residual hazards.

These hazards can be avoided through strict observance of our safety information.

2.1 Proper use

- Easy to use device for quickly measuring the relative air humidity of stacks of cardboard and paper and for determining the residual humidity of diverse materials
- Easy to use device for automatic climate monitoring of printing rooms or storage rooms

2.2 Improper use

- The device must not be used in ATEX.
- The device is not waterproof and must be protected from water and fine dust.

2.3 User qualifications

The device must only be operated by people who can be expected to reliably take the measurements. The device must not be operated by people whose reaction times may be slowed due to, e.g. the use of drugs, alcohol or medication.

All persons using this device must have read, understood and follow the instructions provided in the operating manual.

2.4 General safety information

The following safety information has to be observed at all times to avoid damage to objects and injury to people:

- Remove the batteries if the device isn't used for a prolonged period of time (4 weeks).
- In case of damages or loose parts on the device, remove the batteries and contact Schaller GmbH or your dealer.

All of the device's technical features have been inspected and tested before delivery. Every device has a serial number. Do not remove the tag with the serial number.

2.5 Warranty

The warranty does not apply to:

- Damage resulting from non-observance of the operating manual
- Damage resulting from third-party interventions
- Products that have been used improperly or modified without authorisation
- Products with missing or damaged warranty seals
- Damage resulting from force majeure, natural disasters, etc.
- Damage from improper cleaning
- Batteries older than six months

3. On receipt of your device

3.1 Taking the device out of its packaging

- Take the device out of its packaging.
- Next, make sure that it is not damaged and that no parts are missing.

3.2 Making sure that all of the components have been included

Make sure that all of the components have been included by checking the package contents against the following list:

- humimeter RH6
- 4 pieces of AA Alkaline batteries
- Rubber protection cover

- humimeter USB data interface module - USB stick with software and USB cable
- Wooden case
- Operating manual

Optional accessories:

- Sword sensor holder - for protecting the sword sensor in heavy material stacks
- Tool for removing the sword sensor holder - from heavy material stacks
- Calibration equipment and calibration ampoules - for checking the calibration of the humimeter RHx series
- Battery operated portable thermal printer (only possible together with humimeter USB data interface module) - described in a separate operating manual
- Bluetooth module - described in a separate operating manual


3.3 Inserting batteries

1. Remove the rubber protection cover. To do so, hold the rubber protection cover at the upper side and pull it over. Remove the protection cap of the USB socket beforehand (figure 1 and 2).
2. Take hold of the device with one hand, press your thumb onto the engraved area of the battery compartment (1) and drag downwards (2) (figure 3).
3. Insert the batteries with negative and positive terminals matching those indicated on the battery compartment. Press down the batteries so that they lay flat on the bottom of the housing (figure 4).
 - » As soon as all batteries have been inserted, the device switches on automatically.
4. Push the battery cover onto the housing until it clicks into place (figure 5). Then mount the rubber protection cover onto the housing, beginning at the end where the battery compartment is situated.



4. Using the device - Basics

4.1 Switching the device on




- Press the  button for 3 seconds.
 - » The display will then show the status indicator (see "9. Checking the device's status").
 - » After inserting the batteries, the device switches on automatically.


4.2 Selecting the product type

To do so: The device has to be in the product selection menu.

For an overview of the different product types and the criteria for selecting them, please refer to "7. Product types".

Press the  or  button to move from one product to the next Or

1. Press the  or  button for 2 seconds to open the product type overview. (figure 6).
 - » All product types that are enabled for your device type are displayed in black and can be selected.
2. Use the arrow keys to move from one product type to the next
3. and keep any of them pressed to scroll through the types.
4. Confirm your selection by pressing .
 - » The product type you selected will now be shown at the top of the display.



4.3 Taking a measurement

- For information on how to take a measurement, see section "5. The measuring process".

4.4 Switching the device off




To do so: The device has to be in the product selection or Data Log menu. It is not possible to switch off the device when it is in the main menu.

- Press the  button for 2 seconds.

5. The measuring process

5.1 Taking a measuring at a stack

To do so: Let your humimeter device adjust to the surrounding temperature of the product being measured before the measurement (see ["5.2 Adjustment behaviour of the sensor"](#)).

1. Take hold of the device with one hand and insert the sword sensor 10 cm into the stack (figure 7).
 
- » Make sure to push the sword sensor straight into the stack to prevent a bending of the aluminium sword.
 
- » In case of heavy stacks, use the optionally available sword sensor holder and the tool for removing the sword sensor holder (figure 8).
2. Push the sword a few centimetres further into the stack at short intervals (approx. 10 seconds) (figure 9).
 
3. Let the device adjust to the material being measured for an adequate time period (see ["5.2 Adjustment behaviour of the sensor"](#)).
4. Now take the measured values shown on the display of the device.
 - » Once the reading has been taken, it can be saved on the device (see ["6.2 Saving your readings manually"](#) or ["6.3 Auto save function \(time-based\)"](#)).



ATTENTION

Damage to the aluminium sword

The aluminium sword can be bent by pushing it in or out at an angle.

- Push the aluminium sword straight into the material and pull it straight out of the material.

5.1.1 Taking a measurement of single pieces

To do so: Tight packaging material required. Let your humimeter device adjust to the surrounding temperature of the product being measured before the measurement (see ["5.2 Adjustment behaviour of the sensor"](#)).

1. Put the material being measured into the packaging (figure 10).
2. Take hold of the device with one hand and insert the sword into the packaging so that it is completely enclosed by the material.
3. Seal the packaging to prevent air exchange with the environment (figure 11).
4. Let the device adjust to the material being measured for an adequate time period (see ["5.2 Adjustment behaviour of the sensor"](#)) (figure 12).
5. Now take the measured values shown on the display of the device.
 - » Once the reading has been taken, it can be saved on the device (see ["6.2 Saving your readings manually"](#) or ["6.3 Auto save function \(time-based\)"](#)).



i Information - Measuring accuracy

This rapid and non-destructive measuring procedure allows you to take moisture readings at a number of different points. When saving the individual readings, the device will automatically calculate the readings' average (see ["6.2.2 Saving several readings \(a measurement series\) at the same time"](#)).


i Information - Incorrect readings

Always make sure to select the correct product type for the material you are measuring. This prevents taking incorrect readings (see ["13. Faults"](#)).

5.2 Adjustment behaviour of the sensor

In humidity and temperature measurement, several parameters are responsible for the adjustment behaviour (time until the actual measuring value is displayed). The parameter responsible for the highest measuring error is a temperature discrepancy between the sensor resp. the whole measuring instrument and the material being measured resp. the air.

Therefore, allow your humimeter device to adjust until the displayed temperature corresponds to the actual temperature. The graph below shows how long it takes to adjust from 20 °C to 30 °C:

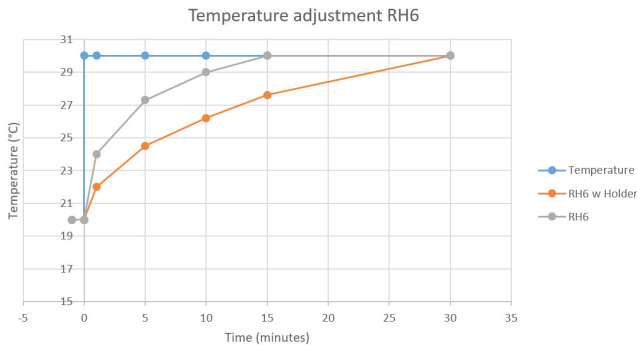

When using the sword sensor holder, pay attention to the temperature adjustment between the sword sensor holder and the sword.

To demonstrate the importance of temperature adjustment, the table below shows the measuring errors due to a temperature difference between the measuring instrument and the material being measured of only 1 °C / 1.8 °F, at different ambient temperatures.

	10 °C (50 °F)	20 °C (68 °F)	30 °C (86 °F)
10 % r.h.	+/- 0.7 %	+/- 0.6 %	+/- 0.6 %
50 % r.h.	+/- 3.5 %	+/- 3.2 %	+/- 3.0 %
90 % r.h.	+/- 6.3 %	+/- 5.7 %	+/- 5.4 %

At room temperature (20 °C / 68 °F) and an assumed paper moisture value of 50 % r.h. a temperature difference between the measuring sensor and the material being measured of 1 °C / 1.8 °F causes a measurement error of 3.2 % r.h. A temperature difference of 3 °C / 5.4 °F would cause a measurement error of more than 10 % relative humidity.













6. Saving your readings



6.1 Hold function - Freezing the displayed values

The device can be configured in such a way that the information being shown on the display will freeze at the touch of a button until a new button is pressed. This function can be very useful when e.g. taking readings in spaces where it is not possible to see the display (e.g. overhead).

6.1.1 Activating the Hold function in the Options menu



To do so: The device has to be switched on and be in the product selection menu.


1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Log Time** (figure 13). To do so, press  or  and confirm by pressing .
4. Select **Hold** (figure 14). To do so, press  or  and confirm by pressing .
 - » The setting has been saved.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.



6.1.2 Using the Hold function


To do so: The device has to be switched on and be in the Data Log menu.

- Press .
- » The current reading will be frozen. All of the four symbols will now be displayed as  (figure 15).
- To reactivate the frozen display, simply press any button.



6.2 Saving your readings manually

All of the readings can be saved, edited and viewed on the device. The figure below shows the overview screen of a single saved series of measurements.

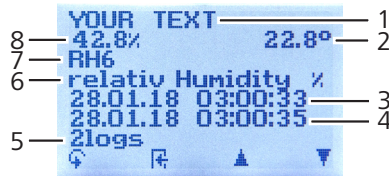











No.	Name
1	Name of the measurement series (editable)
2	Temperature (average)
3	Date & start time of the measurement series
4	Date & end time of the measurement series
5	Number of saved readings
6	Product type
7	Device name
8	Relative air humidity (average)


6.2.1 Saving individual readings



The device can be configured in such a way that the device will save a reading every time a button is pressed. This option (manual save function) is the device's default setting.

Activating the manual save function in the Options menu

To do so: The device has to be switched on and be in the product selection menu.











1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Log Time**. To do so, press  or  and confirm by pressing .
4. Select **Manual** (figure 16). To do so, press  or  and confirm by pressing .





- » The setting has been saved.
- 5. Press  to leave the **Options** menu.
- 6. Press  to leave the main menu.

Using the manual save function



To do so: The device has to be in the Data Log menu (see "Data Log menu" page 5).


1. Press .
 - » The display will now appear as shown in figure 17 and the measured value will be preceded by the digit one.
2. Press  to enter a name for the saved reading and to finish the measuring process.
 - » The display will now appear as shown in figure 18.
3. The data you have inputted can be overwritten at any time.
4. **Inputting letters:**
Press and hold  to quickly scroll to the required letter and either press it for 3 seconds or press  to confirm the selected letter (figure 19).
5. **Inputting numbers:**
Press and hold  to quickly scroll to the required number and either press it for 3 seconds or press  to confirm the selected number.
6. **Moving forward/back:**
Press  to switch to another input level. Press  or  to move forward or back.
7. Confirm your entry by pressing .
 - » The data you entered has been saved




6.2.2 Saving several readings (a measurement series) at the same time



To do so: The device has to be in the Data Log menu (see "Data Log menu" page 5).


1. Take several readings (see "5. The measuring process").
2. To save a reading, press  as soon as the reading has been taken.
3. The display will now appear as shown in figure 20. The marked number shows the number of readings that have already been saved.
4. Press  to enter a name for the saved reading and to finish the measuring process.






5. The display will now appear as shown in figure 21.
6. The data you have inputted can be overwritten at any time.







7. **Inputting letters:**
Press and hold  to quickly scroll to the required letter and either press it for 3 seconds or press  to confirm the selected letter (figure 22).



8. **Inputting numbers:**
Press and hold  to quickly scroll to the required number and either press it for 3 seconds or press  to confirm the selected number.



9. **Moving forward/back:**
Press  to switch to another input level. Press  or  to move forward or back.













10. Confirm your entry by pressing .
 - » The data you entered has been saved.



6.3 Auto save function (time-based)

The device can be configured in such a way that it will automatically save a reading (log) at a selected time interval.

6.3.1 Activating the Auto save function in the Options menu



To do so: The device has to be switched on and be in the product selection menu.



1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Log Time** (figure 24). To do so, press  or  and confirm by pressing .
4. Navigate to the desired time interval (figure 25). To do so, press  or  and confirm by pressing .
 - » The setting has been saved.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.



6.3.2 Auto save function: Saving measured values

To do so: The device has to be in the Data Log menu (see "Data Log menu" page 5).

1. Press .
 - » The device will save a reading at the selected time interval. The number of data saves will increase by one every time a reading is saved. The display will now appear as shown in figure 26.
2. Press  to finish the measuring process and to enter a name for the saved readings.
 - » The display will now appear as shown in figure 27.
3. The data you have inputted can be overwritten at any time.




4. **Inputting letters:**
Press and hold **A..Z** to quickly scroll to the required letter and either press it for 3 seconds or press **↵** to confirm the selected letter.
5. **Inputting numbers:**
Press and hold **0..9** to quickly scroll to the required number and either press it for 3 seconds or press **↵** to confirm the selected number.
6. **Moving forward/back:**
Press **↕** to switch to another input level. Press **➡** or **⬅** to move forward or back.
7. Confirm your entry by pressing **↵**.
 - » The data you entered has been saved.

6.4 Viewing individual readings








To do so: You must have saved a reading (e.g. **1 log**). The display will now appear as shown in figure 28.




1. Press **📊**.
2. Select the required reading. To do so, press **📉** or **📈**.
 - » The display will now appear as shown in figure 29
 - » Press **🏠** to leave this screen.



6.5 Viewing individual readings from a series of measurements









To do so: You must have saved a series of measurements (e.g. **2 logs**). The display will now appear as shown in figure 30.



1. Press .
2. Navigate to the required measurement series. To do so, press  or .
 - » The display will now appear as shown in figure 31.
3. Press  to switch to another input level.
 - » The display will now appear as shown in figure 32.
4. Press  again.
 - » The display will now appear as shown in figure 33.
5. Navigate to the required reading (**No.: 1, No.: 2, No.: 3**). To do so, press .
6. Press  to leave this screen.





6.6 Deleting all measured values (data log)

To do so: You must have taken and saved one or several readings.







1. Press  twice or hold for 2 seconds.
2. Select **Edit Logs** (figure 34). To do so, press  or  and confirm by pressing .
3. Select **Clear Logs** (figure 35). To do so, press  or  and confirm by pressing .
4. The display will then show the message **clear?** (figure 36).
5. Confirm by pressing .
 - » The data log has been deleted.







6. Press  to leave the **Edit Logs** menu.
7. Press  to leave the main menu.

6.7 Deleting individual measurement series











To do so: You must have saved a measured value (e.g. **1 log**) or a series of measurements (e.g. **3 logs**). The display will now appear as shown in figure 37.







1. Press .
2. Select the required reading. To do so, press  or .
 - » The display will now appear as shown in figure 38.
3. Press  to switch to another input level.
 - » The display will now appear as shown in figure 39.
4. Press .
 - » The display will then show the message **clear?** (figure 40).
5. Confirm by pressing .
 - » The value has been deleted.



6.8 Deleting individual values from a single series of measurements

To do so: You must have saved a series of measurements comprising at least 2 logs. The display will now appear as shown in figure 41.

1. Press .
2. Select the required reading. To do so, press  or .
 - » The display will now appear as shown in figure 42.
3. Press  to switch to another input level.
 - » The display will now appear as shown in figure 43.
4. Press .
5. The display will now appear as shown in figure 44.
6. Select the required measured value. To do so, press  or .
7. Press  to switch to another input level.
 - » The display will now appear as shown in figure 45.
8. Press  to delete the value shown.
 - » The display will then show the message **clear?** (figure 46).
9. Confirm by pressing .
 - » The value has been deleted.
 - » Also deleted measuring values will be transferred to the LogMemorizer (see "8. Using the LogMemorizer program") and have to be deleted separately there.



7. Product types

Product type	Definition	Unit	Measuring range
Absolute Humidity	absolute air humidity	g/m ³	0 to 130 g/m ³
Dew Point	Dew Point	°C °F	-55 °C to +60 °C -67 °F to 140 °F
Relativ Humidity	relative air humidity	% RH	0 to 100 %
EMC Wood	Wood equilibrium moisture content (EMC)	% Ugl.	2 to 30 % (wood moisture)
aH Powerliner %	Absolute humidity of Powerliner paper	%	5 to 15 %
aH testliner %	Absolute humidity of Testliner paper	%	3 to 12.2 %
Empty 1 - 5	free calibration curves for special products		

7.1 Definition product types

Absolute humidity

The absolute air humidity shows the contained amount of water in gramme per cubic metre of air. The absolute humidity is a direct degree for the amount of water vapour contained in a certain air volume. It shows how much condensate can precipitate or how much water has to be evaporated in order to obtain the desired humidity.

Dew Point

The dew point is the temperature to which the air that is not completely saturated with water vapour must be cooled so that it is completely saturated. When a room with the current relative humidity cools down to the dew point temperature, the water vapour begins to condense.

Relative humidity

Indicates the relationship between the current water vapour pressure and the maximum possible, the so-called saturation vapour pressure.

The relative humidity shows the degree the air is saturated with water vapour.
Examples:

50% relative humidity: At the current temperature and pressure, the air is half saturated with water vapour. 100% relative humidity means that the air is totally saturated with water vapour. If the air has more than 100% humidity, the excessive humidity would condense or precipitate as mist.

EMC wood

Shows the wood equilibrium moisture content (for wood stored under these conditions) in % wood moisture and the temperature in the selected unit (°C or °F).

aH Powerliner

Shows the equilibrium moisture content of Powerliner paper (for paper stored under these conditions) in % moisture content and the temperature in the selected unit (°C or °F).

aH testliner

Shows the equilibrium moisture content of Testliner paper (for paper stored under these conditions) in % moisture content and the temperature in the selected unit (°C or °F).


Empty 1-5

They can be used for measuring special products (temperature compensated).

The creation of customer specific calibration curves is described in a separate operating manual. On request Schaller GmbH can develop customer-specific calibration curves for your product.

7.2 Application range


Within the normal application range (normal range) the accuracy of the device is as indicated. A long-term application beyond the normal application range (max. range), particularly at an air humidity of more than 80%, can lead to higher measuring errors (+3 % after 60 hours). Back in the normal application range, the sensor will return to the indicated accuracy automatically.

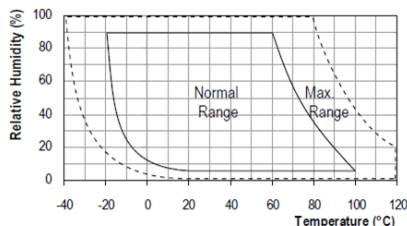

8. Using the LogMemorizer program

8.1 Installing/Opening the program

1. Insert the USB stick with the LogMemorizer program into the USB port on your computer.
2. Open the **setup** application.
3. Follow the installation instructions.
4. Open LogMemorizer.
 - » The screen will now display the LogMemorizer's interface (figure 47).
 - » Before using LogMemorizer, please refer to the the separate LogMemorizer operating manual for the correct configuration of the USB COM Port.

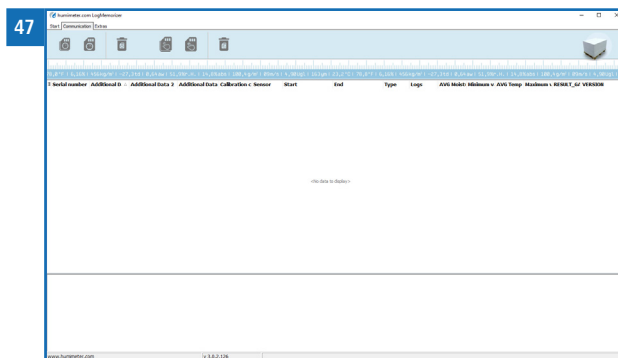

For more information on LogMemorizer, please refer to the separate LogMemorizer operating manual supplied with the device.








8.2 Exporting measured values to a computer



To do so: LogMemorizer must be installed. And you must have taken and saved one or several moisture readings.

Options: You can export moisture readings from the humimeter RH6 or initiate the export at your computer.

Exporting moisture readings from the humimeter RH6

Connect the humimeter RH6 to your computer using the supplied USB cable.


1. Insert the USB Mini B connector into the humimeter RH6 (figure 48).
2. Insert the USB connector into the computer.
3. Open LogMemorizer on your computer.
4. Switch on the humimeter RH6.
5. Press  twice or hold for 2 seconds.
6. Select **Send Logs** (figure 49). To do so, press  or  and confirm by pressing .
7. Select **Manual Logs** or **Auto Logs** (figure 50). To do so, press  or  and confirm by pressing .
8. The display will then show the message **Send** (figure 51).
 - » All of the measuring values saved on the humimeter RH6 will now be sent to your computer.




Initiating the data export at your computer

Connect the humimeter RH6 to your computer using the supplied USB cable.

1. Insert the USB Mini B connector into the humimeter RH6 (figure 52).
2. Insert the USB connector into the computer.
3. Open LogMemorizer on your computer.
4. Switch on the humimeter RH6.
5. Open the **Communication** tab in LogMemorizer (figure 53).

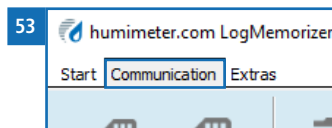



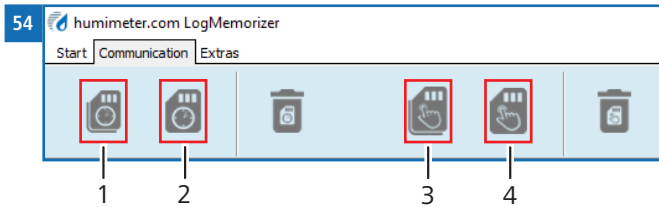

6. Select and click on one of the buttons shown in **figure 54**:
- » **Import all manual logs** (for importing all manually saved readings)
 - » **Import most recent manual log** (for importing the most recent manually saved logs)
 - » **Import all auto save logs** (for importing all auto save readings)
 - » **Import most recent auto save log** (for importing the most recent auto save logs).




No.	Name
1	Import all auto save logs
2	Import most recent auto save series
3	Import all manual logs
4	Import most recent manual log



- » The measuring values saved on the humimeter RH6 will now be sent to your computer.

9. Checking the device's status

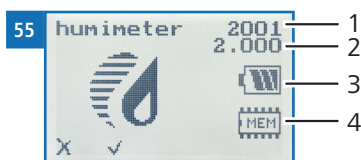1. Press  twice or hold for 2 seconds.
2. Select **Status**. To do so, press  or  and confirm by pressing .
 - » The display will then show the status indicator **humimeter**.
 - » The display will show the following information (figure 55):



No.	Name
1	Serial number
2	Software version
3	Battery status
4	Memory status








3. Confirm by pressing .
4. Press  to leave the main menu.

10. Configuring the device


10.1 Turning on Bluetooth

The information on Bluetooth is provided in a separate operating manual.


10.2 Adjusting the date/time


1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Date/Time**. To do so, press  or  and confirm by pressing .

- » The display will now appear as shown in figure 56.
- » The format for the date is **DD-MM-YY** (Day-Month-Year).
- » The format for the time is **hh:mm:ss** (hour:minutes:seconds).



4. Inputting numbers:



Press and hold **0..9** to quickly scroll to the required number and either press it for 3 seconds or press  to confirm the selected number (figure 57).



5. Moving forward:

To move forward between **DD-MM-YY** and **hh:mm:ss**, press .

6. Moving back:

Press  to switch to another input level. To move backward between **DD-MM-YY** and **hh:mm:ss**, press .

7. Confirm the date/time by pressing **OK**.

- » The settings have been saved.

8. Press to leave the **Options** menu.

9. Press to leave the main menu.

10.3 Selecting a language

1. Press twice or hold for 2 seconds.

2. Select **Options**. To do so, press or and confirm by pressing .

3. Select **Language**. To do so, press or and confirm by pressing .

4. Navigate to the required language. To do so, press or and confirm by pressing .















- » The setting has been saved.



5. Press to leave the **Options** menu.

6. Press to leave the main menu.

10.4 Activating options

To do so: Some of the options must be deactivated.

1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Unlock**. To do so, press  or  and confirm by pressing .
 - » The display will now appear as shown in figure 58.
 - » On delivery, the four-digit password is the device's serial number.
4. **Inputting numbers:**
 Press and hold  to quickly scroll to the required number and either press it for 3 seconds or press  to confirm the selected number (figure 59).
5. **Moving back:**
 Press  to switch to another input level.
 To move back, press .
6. Confirm the four-digit password by pressing .
 - » The setting has been saved.
 - » The °C/°F, BL On Time, Auto OFF Time, Calibrate, Materialcalibration, Online Send, Password, Reset options are now activated.
7. Press  to leave the **Options** menu.
8. Press  to leave the main menu.















10.5 Deactivating options

Once the device has been switched restarted, the **°C/°F**, **BL On Time**, **Auto OFF Time**, **Calibrate**, **Materialcalibration**, **Online Send**, **Password**, **Reset** options will be deactivated again.

10.6 Selecting °C/°F













To do so: All of the options must be activated (see "10.4 Activating options").

1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **°C/°F**. To do so, press  or  and confirm by pressing .
4. Navigate to the required temperature scale, i.e. Celsius (°C) or Fahrenheit (°F).
To do so, press  or  and confirm by pressing .
- » The setting has been saved.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.

10.7 Reducing the device's power consumption













10.7.1 Configuring the display illumination time

To do so: All of the options must be activated (see "10.4 Activating options").

1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **BL On Time**. To do so, press  or  and confirm by pressing .
4. Select the required display illumination period (30 seconds, 2 minutes, 5 minutes, 10 minutes). To do so, press  or  and confirm by pressing .
- » The setting has been saved.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.

10.7.2 Configuring automatic switch-off

To do so: All of the options must be activated (see "10.4 Activating options").

1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Auto Off Time**. To do so, press  or  and confirm by pressing .
4. Select the period of time you want the device to stay switched on (3 minutes, 5 minutes, 10 minutes). To do so, press  or  and confirm by pressing .
 - » The setting has been saved.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.

10.8 Calibrating the device









For information on how to calibrate your device, see section "12. 2-point (optionally 3-point) calibration".





10.9 Configuring the material calibration function

The type calibration function is described in a separate operating manual.

10.10 Changing the password









To do so: All of the options must be activated (see "10.4 Activating options").



1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Password**. To do so, press  or  and confirm by pressing .
 - » The display will show the current password.
4. Overwrite the current password. To do so, press and hold **0..9** to quickly scroll to the required number and either press it for 3 seconds or press  to confirm the selected number.

5. **Moving back:**
Press  to switch to another input level.
To move back, press .
6. Confirm the new four-digit password by pressing **OK**.
 - » The setting has been saved.
7. Press  to leave the **Options** menu.
8. Press  to leave the main menu.

10.11 Resetting the device to its factory settings

To do so: All of the options must be activated (see "10.4 Activating options").

1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Reset**. To do so, press  or  and confirm by pressing .
 - » The display will then show the message **Reset?** (figure 60).
4. Confirm by pressing .
 - » The device will now be reset to its factory settings. All of your personal settings will be lost.
 - » The display will show the status indicator **humi-meter** (figure 61).
 - » Resetting the device will not affect the saved measuring values.



11. Cleaning and maintenance

Regularly cleaning and maintaining the device will ensure that it will have a long service life and stay in good condition.

11.1 Changing the batteries

The device constantly monitors the charge level of the batteries. The current battery status is shown on the status screen.

If the battery's charge is very low, the battery symbol will be shown with an exclamation mark. In that case, the batteries must be changed immediately (figure 62).

For changing the batteries, see section "3.3 Inserting batteries".

As the device's user, you are responsible by law for properly disposing of all used batteries, which must not be disposed of as domestic waste (Battery Directive).



11.2 Care instructions

- Do not leave the device out in the rain. The device is not waterproof.
- Do not immerse the sensor in water.
- Do not expose the device to extreme temperatures.
- Protect the device from strong mechanical shocks and loads.

11.3 Cleaning the device



ATTENTION

Do not clean with fluids

Water or cleaning fluid getting inside the device can destroy the device.

- Only clean with dry materials.

Plastic housing and sword sensor

Clean the plastic housing and the sword sensor with a dry cloth.

Air humidity and temperature sensor




The air humidity and temperature sensor cannot be cleaned. In case of a polluted sensor please contact your dealer.

12. 2-point (optionally 3-point) calibration

To do so: Calibration equipment (art.no.10072) and calibration ampoules (humidity standards art.no.10005) required. The device, the calibration equipment and the humidity standards must have a temperature between 20.0 °C and 26.0 °C. It is recommended to store the device, the calibration equipment and the calibration ampoules in a room with little temperature fluctuation for 24 hours.

12.1 Assembling the calibration equipment

1. Insert the first sealing ring (1) (figure 64) into the upper part of the calibration equipment (figure 65).
2. Insert the sword sensor into the upper part of the calibration equipment (figure 66).
3. Insert the second sealing ring (2) (figure 64) into the upper part of the calibration equipment (figure 67).
4. Put the textile pad in the lower part (figure 68) and carefully pour the humidity standard onto the pad, beginning with the humidity standard of 35 % relative humidity.
5. Put the third sealing ring (4) (figure 64) onto the lower part (figure 69), then put the aluminium disc (3) onto it (figure 64).
6. Carefully place the upper part together with the RH6 sword probe on the lower part (figure 70).
7. Recommendation: First screw the lower part lying on the table counterclockwise into the upper part and lift it straight to complete the screwing.
 - » Take care to lift the RH6 device with calibration equipment straight up and not to tilt or turn it over. Otherwise the sensor may be damaged.

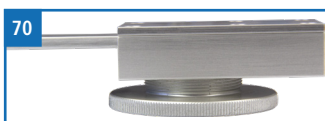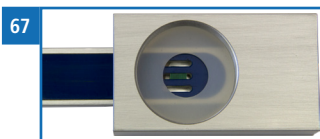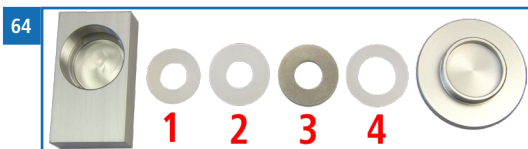

8. Carefully place the RH6 device with calibration equipment on a table.
 - » Leave the calibration equipment mounted on the sword probe until explicitly stated otherwise.



ATTENTION

Damage to the sensor

By tilting or turning the device with mounted calibration equipment the sensor can be destroyed.

- Only lift the device with mounted calibration equipment straight up.

12.2 Determining the deviation

1. Let the sensor adjust to the humidity standard for at least 2 hours.
2. Then note down the measured relative humidity and temperature.
3. At ideal temperature conditions (device, calibration equipment and humidity standard have a temperature of 23 °C), the value printed on the humidity standard can be used as reference value.
4. In case of deviation from the factory temperature (23.0 °C), the real humidity value must first be determined according to the table below.

Temperature	Humidity standards		
	35 %	50 %	80 %
20 °C	34.6%	49.8%	79.9%
21 °C	34.8%	49.8%	80.0%
22 °C	34.9%	49.9%	80.0%
23 °C	35.0%	50.0%	80.0%
24 °C	35.1%	50.1%	80.0%
25 °C	35.2%	50.2%	80.0%
26 °C	35.4%	50.2%	80.1%

5. Note down the real humidity value.
6. Compare the noted displayed measuring value with the real humidity value.
 - » If the deviation revealed is below 1.5 % relative humidity, it is not recommended to recalibrate. In this case, remove the calibration equipment from the sword probe.















- » If the deviation revealed is more than 1.5 % relative humidity, it is recommended to perform a recalibration.


12.3 Performing a recalibration

To do so: The deviation revealed is more than 1.5% relative air humidity. All of the options must be activated (see "10.4 Activating options").

12.3.1 Determination of calibration values


To do so: Microsoft Excel calculation sheet required (available via email, on request by phone or by email to support@schaller-gmbh.at).

1. Press  twice or hold for 2 seconds.
 2. Select **Options**. To do so, press  or  and confirm by pressing .
 3. Select **Calibrate**. To do so, press  or  and confirm by pressing .
 4. Select **Humidity**. To do so, press  or  and confirm by pressing .
- » The display will then show the first index, Index1 (Idx:[1]) (figure 71).
5. Enter the indices 1 to 6 of the Ic values already stored in the device into the corresponding fields of the MS Excel calculation sheet, paying attention to the volt values (figure 72). Navigate through the indices by pressing  twice until you have returned to Index1 (Idx:[1]).
 6. Press .
 7. The Ic value (upper line) has to change (figure 73).
 - » If Index7 (Idx:[7]) is displayed after the key is released, the key has been pressed too long.
 - » In that case navigate back to Index1 (Idx:[1]) by pressing  and press  shorter.



72

Factory calibration values		
	IC-Values	V-Values
Idx [1]	16 383 Ic	4,785 V
Idx [2]	11 180 Ic	3,380 V
Idx [3]	7 220 Ic	2,300 V
Idx [4]	5 274 Ic	1,760 V
Idx [5]	2 400 Ic	0,896 V
Idx [6]	1 086 Ic	0,500 V



8. Now enter the real humidity value, the temperature, the displayed humidity value and the new Ic value (point 7) of the humidity standard 35% relative humidity into the corresponding fields in the MS Excel calculation sheet (figure 74).











74


	Determined calibration values			
	real humidity	shown temperature	shown relative humidity	assumed IC-values
at approx. 35%	35,0%			5 637 Ic
at approx. 50%	50,0%			7 600 Ic
at approx. 80%	80,0%			11 128 Ic

- » If you forget to enter one value, the calculation is wrong.
9. Now do not press any other key on the device and wait until it switches itself off (by default this takes about 5 minutes).
- » Up to this point, no changes have been made to the calibration.
10. Now remove the calibration equipment from the sword probe and repeat the procedure from "12.1 Assembling the calibration equipment", optionally with the humidity standard 50 % relative humidity or the humidity standard 80 % relative humidity.

12.3.2 Entering the calculated calibration values into the RH6

To do so: The Microsoft Excel calculation sheet has been filled in correctly.

1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Calibrate**. To do so, press  or  and confirm by pressing .
4. Select **Humidity**. To do so, press  or  and confirm by pressing .
- » The display will then show the first index, Index1 (Idx:[1]) (figure 75).



5. Overwrite the current Ic-value with the new calculated Ic-value for this index (figure 76). To do so, press and hold **0..9** to quickly scroll to the required number and either press it for 3 seconds or press **↵** to confirm the selected number (figure 77).

76

new calibration values		
	IC-Values	V-Values
Idx [1]	15 971 Ic	4,785 V
Idx [2]	11 128 Ic	3,380 V
Idx [3]	7 445 Ic	2,300 V
Idx [4]	5 637 Ic	1,760 V
Idx [5]	2 708 Ic	0,896 V
Idx [6]	1 772 Ic	0,500 V

Moving back:

Press **↑** to switch to another input level.

To move back, press **←**.

77

RH6 Humidity		01284567
Idx:[1]	16100 Ic	
	4.100V	
↑	↵	0..9 V

6. Navigate to the next index by pressing **↵** twice.
7. Repeat steps 5 and 6 for the rest of the calculated indices, leaving index7 (Idx:[7]) untouched.
8. Press **↑** to switch to another input level and **↵** to leave the **Humidity** menu.
 - » The recalibration has been saved.
9. Press **↵** to leave the **Calibrate** menu.
10. Press **↵** to leave the **Options** menu.
11. Press **↵** to leave the main menu.
12. In case of an incorrect recalibration, it is possible to reset the device to its factory settings (see "10.11 Resetting the device to its factory settings").
 - » By restoring the factory calibration, recalibrations that have already been carried out successfully are deleted.

13. Faults

If the measures listed below fail to remedy any faults or if the device has faults not listed here, please contact Schaller GmbH.

Fault	Cause	Remedy
Measuring error	The temperature of the material being measured is too low or high. I.e. the material's temperature is lower than -10 °C or higher than +60 °C	The temperature of the material being measured has to be between -10 °C and +60 °C.
	Measurement error due to too short temperature adjustment time	Let the temperature adjust to the material being measured (see "5.2 Adjustment behaviour of the sensor").
	Wrong product type	Check whether you have selected the right product type (product) before taking a reading (see "7. Product types").
	Dripping water or sprayed water	Direct contact of the sensor with dripping or sprayed water will destroy it.
	Irreversible damage of the sensor due to aggressive gases	Please contact your dealer.
	Condensation caused by a change in temperature	Condensation on the sensor interferes with the calibration. Let the device adjust to the surrounding temperature.
	Polluted air humidity and temperature sensor	Please contact your dealer.
	Foreign particles on the sensor	Please contact your dealer.
Data transfer to Log-Memorizer failed	Interface has not been configured	The interface only has to be configured once. To do so, press the F1 key on your computer and read the Help file for your LogMemorizer program.


14. Storage and disposal

14.1 Storing the device

The device must be stored as follows:

- Do not store outdoors.
- Store in a dry and dust-free place.
- Protect the device from sunlight.
- Avoid mechanical shocks/loads.
- Remove the batteries if the device is not used for a period of 4 weeks or longer.
- Storage temperature: -20 °C to +60 °C.

14.2 Disposing of the device



Devices marked with this symbol are subject to Directive 2012/19/ EU of the European Parliament and of the Council of 4 July 2012 on waste electrical and electronic equipment (WEEE).

If the device is being operated outside the European Union, the national regulations on the disposal of such devices that apply in the country of use must be observed.

Electronic devices must not be disposed of as domestic waste.

The device must be disposed of appropriately using appropriate collection systems.

15. Device information

15.1 EC declaration of conformity

CE DECLARATION OF CONFORMITY

We

Schaller GmbH
Max-Schaller-Straße 99
A – 8181 St. Ruprecht

in accordance with the following Directives:

EMV - Richtlinie 2014/30/EU,
RoHS - Directives 2011/65/EG,

hereby declare that the following product types:

Product: **humimeter**

Types: **RH1 ; RH2 ; RH5 ; RH5.1 ; RH6**

are in conformity with the applicable requirements of the following documents

- **EN 61326–1:2013** Electrical equipment for measurement, control and laboratory use – EMC requirements
- **EN 50581:2012** Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances:

I hereby declare that the equipment named above has been designed to comply with the relevant Sections of the above referenced specifications. The unit complies with all applicable Essential Requirements of the Directives.

St. Ruprecht a.d. Raab, 21.03.2016

Max Schaller

Schaller GmbH
Maximilian Schaller
General Manager

15.2 Technical data

Display resolution	0.1 % rel. air humidity, 0.1 g/m ³ abs. air humidity 0.1 °C/0.3 °F dew point 0.1 °C/0.3 °F temperature 0.1 % EMC Wood
Measuring range relative air humidity	0 % to 100 %
Calibration relative air humidity	10 % to 90 %
Measuring range dew point	-55 °C to +60 °C
Measuring range EMC Wood	2 % to 30 %
Calibration EMC Wood	5 % to 15 %
Accuracy rel. air humidity	+/- 1.5 % (at 25 °C)
Accuracy temperature	+/- 0.3 °C (at 25 °C)/+/- 0.5 °F (at 77 °F)
Accuracy EMC Wood	+/- 0.5 % (at 25 °C)
Operating temperature	-10 °C to +60 °C
Storage temperature	-20 °C to +60 °C
Temperature compensation	Automatic
Data memory	Up to 10,000 measuring values
Power supply	4 pcs. of 1.5 Volt AA Alkaline batteries
Current consumption	60 mA (incl. display illumination)
Menu languages	German, English, French, Italian, Spanish, Portuguese, Czech, Polish, Russian, International
Display	128 x 64 illuminated matrix display
Device dimensions	295 x 64 x 30 mm
Case dimensions	506 x 116 x 50 mm
Device weight	260 g
Weight of device + case	650 g
Device IP rating	IP 40



Climate
Environment



Materials



Food



Buildings



Bioenergy



Paper / Board

Schaller Messtechnik develops, produces and sells professional moisture meters and turnkey solutions.

Schaller GmbH

Max-Schaller-Straße 99, A - 8181 St. Ruprecht an der Raab

Tel +43 (0)3178 - 28899 , Fax +43 (0)3178 - 28899 - 901

info@humimeter.com, www.humimeter.com